

## Instruction manual


### Auto-slide cover test prod MODEL 7313

- How to switch the measurement categories

Applicable measurement categories are switchable between CAT II 1 kV and CAT IV 600 V just by turning the protective cover.

Sliding the protective cover is possible only at CAT II 1 kV.

When using this probe in CAT III or higher environment, turn the protective cover and set it to CAT IV 600 V: visible through the oval window. (Then the protective cover is locked.)

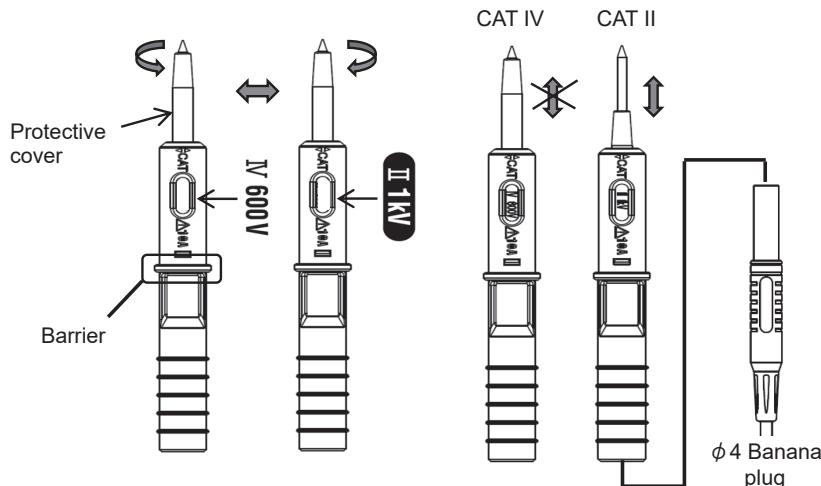

- Combined use with our test leads with φ4 Banana plug is possible. When using commercially available test leads, Kyoritsu assumes no responsibility for damages and injuries resulting from the use of them regardless of the causes or nature of the incidents.

\* When test leads are connected to and used with the instrument, the lower category either of them belongs to is applied.

**△ DANGER**

Barrier is a part providing protection against electrical shock and ensuring the minimum required clearance and creepage distance. Keep your hand and fingers behind the barrier during a measurement.

**△ CAUTION**

Do not apply force to the tip metal part in an unusual direction.



**KYORITSU ELECTRICAL  
INSTRUMENTS WORKS, LTD.**